

An improvised endotrainer for low resource settings

Omokanye LO¹, Olatinwo AWO¹, Salaudeen A G², Balogun OR¹, Saidu R¹

Original Article

Abstract

Training in minimal access surgery has always been difficult in developing countries with limited resources, paucity of animal laboratories, unaffordability/unaffordable conventional endotrainer and limited number of trained endoscopic surgeons to help the trainee.

Objective: To design an endotrainer for use in resource- poor settings with the aim of domestication of laparoscopic surgery.

Materials and Methods: A fabricated endotrainer box with a camera, a bulb for adequate illumination powered by electricity connected to a television was designed at affordable price to improvise for the conventional endotrainer for low resource settings.

Results: The fabricated endotrainer model was found to be an effective training tool for improving psychomotor skills and dexterity of movement, especially for suturing in difficult areas. This is comparable to the sophisticated virtual reality simulator. Also, it is far less expensive compared to the expensive virtual reality simulator, thus affordable.

Conclusion: It is concluded that this model should be employed by other low resource setting to improve the skills of surgeons in endoscopy surgery and facilitate the training of new hands.

Key words; Endotrainer, Minimal access surgery, low resource setting.

Corresponding author; **Dr.Omokanye LO (omostuff1111@yahoo.com)**

¹ Department of Obstetrics and Gynaecology, College of Health Sciences, University of Ilorin

² Department of Epidermiology and Community Medicine, College of Health Sciences, University of Ilorin

Un engin improvisé endotrainer pour faible paramètres de ressource

Omokanye LO¹, Olatinwo AWO¹, Salaudeen UN G², Balogun OR¹, Saidu R¹

L'article d'origine

Résumé

Formation en minimal access surgery a toujours été difficile dans les pays en développement disposant de ressources limitées, le manque de laboratoires animale, inaccessibilité/inabordable endotrainer classiques et d'un nombre limité de formés endoscopique chirurgiens à aider le stagiaire.

Objectif : concevoir un endotrainer pour utilisation en ressource- pauvres paramètres avec l'objectif de la domestication de la chirurgie cœlioscopique.

Matériels et méthodes : fabriquer une endotrainer boîte avec une caméra, une ampoule pour un éclairage alimentés par de l'électricité raccordé à un téléviseur a été conçu à un prix abordable à improviser pour le endotrainer classiques pour les pays qui ont peu de ressources.

Résultats: Les fabriquer soi-même endotrainer modèle a été trouvé pour être efficace un outil de formation pour améliorer leurs compétences psychomotrices et la dextérité du mouvement et surtout de suture dans des zones difficiles. Ceci est comparable à la sophistiquée simulateur de réalité virtuelle. Aussi, il est beaucoup moins coûteux, comparé à la coûteuse simulateur de réalité virtuelle, donc abordable.

Conclusion: il est conclu que ce modèle devrait être employée par d'autres ressources faible réglage pour améliorer les compétences des chirurgiens en chirurgie endoscopique et faciliter la formation de nouvelles mains.

Mots clés; Endotrainer, Minimal Access Surgery, faible paramètre de ressource.

Auteur correspondant: **Dr Omokanye LO (omostuff1111@yahoo.com)**

¹Département d'obstétrique et de gynécologie, Collège des Sciences de la santé, de l'Université d'Ilorin

² Département de Epidermiology et de médecine communautaire, Collège des Sciences de la santé, de l'Université d'Ilorin

INTRODUCTION

Laparoscopy surgery, also referred to as key hole surgery or minimal access surgery is a modern surgical technique in which operations in the abdomen are performed through small incisions (usually 0.5–1.5 cm) as opposed to the larger incisions needed in laparotomy (1). This surgical approach has been used since a century but in the last two decades there has been an explosion in this field. As new technology comes up day by day its indications and applications are also increasing (1).

The advantages of laparoscopy in comparison to open abdominal surgery include reduced surgical trauma, haemorrhage, less pain, fewer post-operative pulmonary complications, and shorter recovery times. The disadvantages include longer surgical times and higher equipment costs and extended training especially in developing nations (2). Adequate training and caution are key points in laparoscopic surgery.

Recognizing the growing role of laparoscopy in modern surgery, residency programs have incorporated it into their training regimen. Various devices ranging from simple box trainers, animal models to sophisticated virtual reality trainers are used to aid in this education of laparoscopic skills. Virtual reality system is an advanced and effective training method, however it is yet to be adopted due to its cost and the advanced technology required for it (3). However formal training in this technique is limited in low resource setting primarily due to high cost of virtual reality simulator and limited numbers of trained endosurgeon (3). We designed an endotrainer for low resource setting to improve the skills of surgeons in the art of endosurgery.

MATERIALS AND METHODS

The endotrainer we have designed is a rectangular box with the dimensions of 35cm x 28cm x 18cm. These dimensions are developed, such that, they nearly correspond to the normal adult peritoneal cavity. This space is adequate for the placement of instruments and training objects. A fabricated rectangular endotrainer box made up of grade A interior plywood with a Color Weather proof IR Closed Circuit Television Camera (CCTV (EC-WC6009) that has in-built light source and a 20 Watt conventional energy saving- white -bulb for adequate illumination powered by electricity and connected to a television via Audio/Video (A/V) cable was designed as an improvisation for virtual reality simulator endotrainer which is expensive for developing nations.

Four holes (5mm each) through which the hand-held laparoscopic instruments are introduced are made in the cover of the box and covered with white rectangular foam to prevent escape of light from within the box which might reduce illumination. The inside of the box simulates an insufflated abdominal cavity and is lined with foam. At the centre, there are two 10cm rectangular foams of equal sizes with a thickness of 0.5cm are held side by side firmly apposed with a gap of 0.5cm was fixed over the white foam covering the floor of the box using Evo-stik gum. This constitutes the working area.

A television stand that houses the 17” television and a trainer box desk (where the endotrainer is placed) are designed specifically for this purpose taken cognizance of the height of the endotrainer and screen position at eye level to ease manipulation. Also, a Light-Emitting Diodes (LEDs) 32” television which displays edited/unedited videos of laparoscopic

surgeries is placed in between the television for demonstration.

Instrument and training

The instruments for endotrainer are similar to those in use for live surgery only that they are made of plastic handle except for needle holder. These include Maryland, babcock, scissors and needle holder. The training pattern in the use of endotrainer is similar to conventional laparoscopic training. Hand-eye coordination, dissection, and suturing exercises are carried out. The hand-eye coordination exercises included transfer of objects between instruments and transfer between petri dish placed within the trainer. The technique of dissection is by cutting round a circle and suturing is practiced using the inner foams.

DISCUSSION

The introduction of laparoscopic surgery in the 1901s brought with it new challenges for the surgeons (4). Previously they looked directly at the target organ through an abdominal wall incision. Now they had to adapt to a new technique in which they had to look at a monitor displaying the intra abdominal scene. As there were no structured instructional courses available it took time for them to adapt to this method of surgery. They needed to acquire excellent hand-eye coordination. Surgeons learning on patients are courting disaster (5). Simulation is the imitation or modeling of a real-life situation for training or instruction. Since the first simplistic endoscopic simulators were described in 1969 (6) and the early 1970s (7, 8), these instruments have evolved greatly over time and now include complex computerized devices.

In the developed world, the finer points for the improvement of the safety of patients undergoing laparoscopic surgery were

debated and guidelines were set. Unfortunately, in developing countries there are no such guidelines and there are only a limited number of trained endosurgeons. The local surgical fraternity was not convinced about the safety of laparoscopic surgery most especially in the developing countries and so a training policy had to be developed which would help to develop hand-eye coordination (3).

Market driven public demand has created unprecedented challenges in training and credentialing within this field. A revolution has occurred in surgical education in the developed world, as a result of availability of virtual reality simulators for the training and assessment of technical skills. This innovation is due to combination of simulators, curriculum-based training, validation of objective assessment and policy (criterion-based bench marks) to deliver high-level proficiency-based training (9). However, the reverse is the case in the developing world where domestication of laparoscopic surgeries is being hampered by the limited resources to procure simulators and lack of trained endoscopic surgeons to help the trainees.

The basic principles of mechanical stimulators have not changed during the last decade; however, it has been constantly upgraded over years (10). The average cost of a standard endotrainer ranges between five thousand to eight thousand five hundred dollars. Due to poor funding of health services this is not within the reach of most developing countries. Therefore, there is need to design an affordable endotrainer in order to initiate and sustain the practice of laparoscopic surgery in these regions. The cost incurred in putting up this model is less than one-sixth (seven fifty dollars) of virtual reality simulators, thus suitable for low-resource setting like ours.

This model operates using the same principles as standard virtual reality

simulators except for some modifications (Fig. 1.). Various tasks as in standard endotrainer like stacking of cube of sugar, cylindrical and dough nut shaped beads on each other, cutting with the aid of endo-scissors round a circle and endo knotting and endo suturing training are being conducted by previously trained endosurgeons (Fig.2, 3, 4, 5, 6). The results are comparable to conventional endotrainer. This is similar to findings of Powers et al and Munz et al in India and United Kingdom respectively (11, 12).

This model is a cost effective training tool for improving psychomotor skills and dexterity of movement, especially for suturing in difficult areas as commonly encountered in minimal access surgical practice. It is therefore recommended to other low resource setting for training and to improve the skills of surgeons who are new to the art of endosurgery.

Conflicts of Interest and Acknowledgment

We appreciate the management of University of Ilorin Teaching hospital for financial assistance rendered to actualize this dream and Maakdatum Engineering Solution, Ilorin, for the design of this model. Also, Apollo Hospital, Chennai; India, Ethicon Institute of Surgical Education, tynampet; Chennai, India and world laparoscopy Hospital, Gurgaon, Delhi; India for training us in laparoscopy

No conflict of interest to be declared.

REFERENCES

1. Stephen W, Eubanks MD. Laparoscopy. In; Steve E, Lee L, Swanstrom MD, Nathaniel JS, editors. *Mastery of Endoscopic and Laparoscopic Surgery*. 2nd edition Lippincott Williams & Wilkins, 2004; p. 22-26.
2. Smith I. Anesthesia for laparoscopy with emphasis on outpatient laparoscopy. *Anesthesiol Clin North Am*. 2001; 19:21-41.
3. Iqbal SM, Mohsin M, Anjum M, Shah A, Tafazul M. A structured training module using an inexpensive endotrainer for improving the performance of trainee surgeons. *Trop Doct*. 2008; 38: 217-218.
4. Martin H, Kowon ST, Langbein S, Kamp S, Axel H, Peter A. Hans Christian Jacobaeus: Inventor of Human Laparoscopy and Thoracoscopy. *J Endo Urol*. 2006; 20(11): 848-850.
5. Keyser EJ, Derossis AM, Antoniuk M, Sigman HH, Fried GM et al. A simplified simulator for training and evaluation of laparoscopic skills. *Surg Endosc* 2000;14:149–53
6. Bhutani MS, Wong RF, Hoffman BJ. Training facilities in gastrointestinal endoscopy: an animal model as an aid to learning endoscopic ultrasound. *Endoscopy* 2006; 38 (9): 932-934.
7. Heinkel VK, Kimmig JM. “Stomach models for training in gastrocamera examination and gastroscopy”. *J Gastroenterol* 2003; 57(1): 8-16.
8. Sorbi D, Vazquez-Sequeiros E, Wiersema MJ. A simple phantom for learning EUS-guided FNA. *Gastrol intest Endosc* 2003; 57 (4): 580-83.
9. Ahlberg G, Enochsson L, Gallagher AG, Hedman L, Hogman C, McClusky DA 3rd, *et al* . Proficiency-based virtual reality training significantly reduces the error rate for residents during their first 10 laparoscopic cholecystectomies. *Am J Surg*

2007; 193:797-804.

10. Rassweiler J, Klein J, Teber D, Schulze M, Frede T. Mechanical simulators for training for laparoscopic surgery in urology. *J Endourol* 2007; 21:252-62.
11. Powers TW, Murayama KM, Toyama. House staff performance is improved by

participation in a laparoscopic skills curriculum. *Am J Surg* 2002;184:626-9

12. Munz Y, Kumar BD, Moorthy K, Bann S, Darzi A. Laparoscopic virtual reality and box trainers; Is one superior to other? *Surg Endosc* 2004;18:485-94 .



Fig 1. Endotrainer Laboratory



Fig. 2 Hand precision (stacking of cube of sugar)



Fig. 3 Hand precision (Stacking of beads)

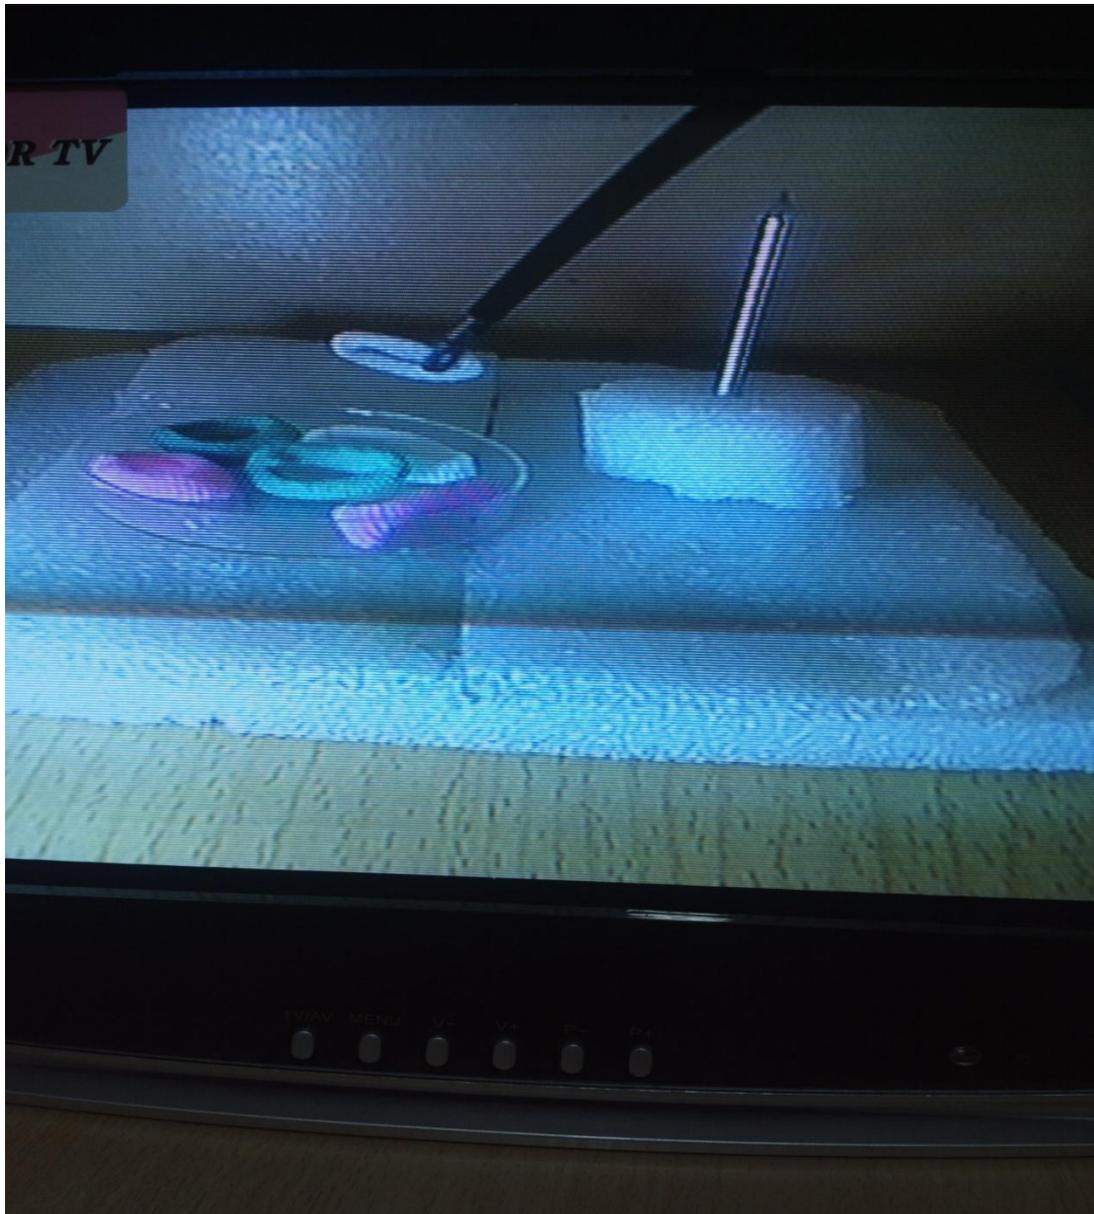


Fig.4 Hand precision (Stacking of Doughnut shaped beads)

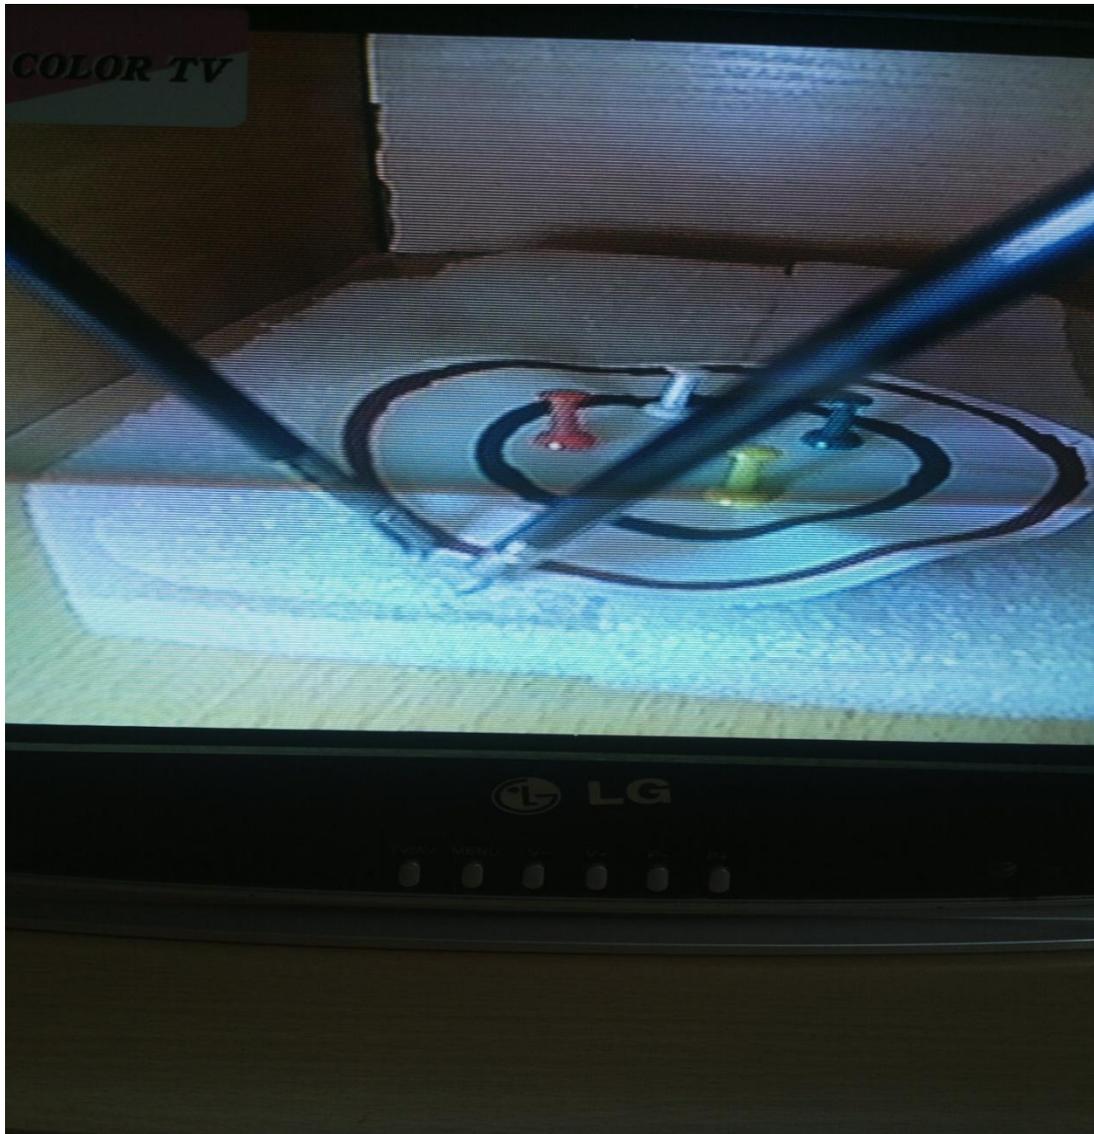


Fig. 5 Dissection precision (Cutting round a circle)



Fig. 6 Suturing precision (Endo-suturing and Knotting)