

A multi-template multiplex PCR assay for hepatitis B virus and human β -globin

Oluwapelumi O. Adeyemi¹  | Morgan R. Herod¹ | Femi Oladiji² |
Yisa M. Fakunle³ | Abiola S. Babatunde⁴ | Olajide O. Agbede⁵

¹ Faculty of Biological Sciences, School of Molecular and Cellular Biology, University of Leeds, Leeds, UK

² Faculty of Clinical Sciences, Department of Epidemiology and Community Health, College of Health Sciences, University of Ilorin, Ilorin, Nigeria

³ Faculty of Clinical Sciences, Department of Medicine, College of Health Sciences, University of Ilorin, Ilorin, Nigeria

⁴ Faculty of Basic Medical Sciences, Department of Haematology, College of Health Sciences, University of Ilorin, Ilorin, Nigeria

⁵ Faculty of Basic Medical Sciences, Department of Medical Microbiology and Parasitology, College of Health Sciences, University of Ilorin, Ilorin, Nigeria

Correspondence

Oluwapelumi O. Adeyemi, Faculty of Biological Sciences, School of Molecular and Cellular Biology, University of Leeds, LS2 9JT Leeds, UK.
Email: bs00a@leeds.ac.uk

Funding information

Tertiary Education Trust Fund (TETFund), Nigeria, Grant number: TETFund/DESS/NRF/20/13/STI/VOL.1

The Hepatitis B surface antigen (HBsAg) is the hallmark of HBV infection. Detection of antibodies to HBs and the core (ie, HBsAg and HBcAb) are primary serological algorithms in the laboratory diagnosis of HBV. Detection of HBsAg DNA is an important supplement to serological diagnosis especially in clinical cases. Simultaneous amplification of internal cellular controls is a good indicator of sample quality. Human β -globin is a well characterized housekeeping gene (HKG) that is often applied as internal controls (IC) in molecular diagnosis. In this study, individual plasmid clones of the human β -globin and HBs genes were constructed. These plasmid constructs have been applied to characterize a multiplex PCR assays for HBs and β -globin genes. The findings suggest detection limits of less than 10 genome copies of either template in vitro using conventional and multiplex PCR conditions. Under the multiplex conditions, co-amplification of β -globin and HBsAg DNA had a resultant effect on assay sensitivity. This study further highlights the importance of molecular diagnosis in HBV infectious individuals. If fully optimized, this assay could provide a possible diagnostic complement to serological detection in developing countries.

KEYWORDS

HBs gene, hepatitis B, housekeeping genes, molecular diagnosis, multiplex polymerase chain reaction, sensitivity

1 | INTRODUCTION

Hepatitis B Virus (HBV) infection is a common cause of chronic hepatitis, liver cirrhosis, and hepatocellular carcinoma which may lead to death.^{1,2} Annually, approximately 4.5 million new cases occur worldwide, 25% of which progress to chronic liver disease. Approximately 5% of the world's populations are chronic carriers with an estimated 620 000 annual deaths as a result of acute and chronic HBV. Although two main vaccines against HBV have been in use for over 3 decades, HBV infections still remain highly endemic in sub-Saharan Africa and East Asia with dire public health concerns.^{3,4}

HBV is an enveloped DNA virus of the family *Hepadnaviridae*. It has a relaxed-circular 3.2 kb genome, which is partially double-stranded (rcDNA). The HBV genome is replicated by reverse transcription of an RNA intermediate. It encodes four overlapping open reading frames that are translated into the viral core protein (C-gene), a highly conserved surface protein (S-gene), the viral polymerase (P-gene), and the X protein (X-gene).⁵ In part, due to the poor fidelity of the viral reverse transcriptase there is broad sequence-variability of the HBV genome with eight main genotypes (A-H) distributed worldwide.⁵⁻⁷ In addition to other possible human genotypes,^{8,9} HBV has also been reported in non-human primates including chimpanzees, woolly

monkeys, orangutans, and gorillas,^{10–12} while non-human HBV-like viruses have been reported in rodents and birds.^{13–15}

Serological and genetic markers are employed as primary algorithms for the screening and diagnosis of various stages and genotypes of HBV infections. The choice diagnostic specimen for HBV infection is the blood and the most significant targets are the viral envelope and capsid.^{16,17} Repeated isolation of the S-antigen (HBsAg) from the blood of infected persons for over 6 months is a diagnostic marker for chronicity, while ongoing infections are diagnosed by the presence of the e-antigen (HBeAg) in the blood.¹⁷ HBV genome quantification in serum or plasma samples is an effective means of measuring viral load over time and remains most informative in diagnosing a carrier state.¹⁸ This has been demonstrated by PCR, which is able to detect less than 10 HBV genome copies/mL of serum or plasma in chronic cases.¹⁷ Despite the high sensitivity of PCR, sensitivity or specificity could be adversely affected by a variety of factors such as poor sample quality or genomic extraction procedures; therefore the application of HKGs as ICs in molecular biology is vital. HKGs are indigenous genes expressed in each cell of an organism under any condition and typically play important roles in many basic cellular functions. There are numerous human HKGs, many of which have been characterized and are often applied as ICs in experimental studies as a result of their consistent levels of expression and high conservation despite infection or other factors.^{19,20} In laboratory and clinical diagnosis, the diagnostic ability of a test is expressed as percentages of real cases that are accurately diagnosed as positive and percentages of non-existent cases that are accurately diagnosed as negative, that is, *sensitivity* and *specificity* of the test. The occurrence of false negative (Type I error) and/or false positive (Type II errors) test results largely determine how effectively an assay could diagnose a condition.^{21,22}

In many developing economies, HBV diagnosis is predominantly serological^{23,24} despite alarming levels of prevalence reported even among blood donors,^{25–28} which suggests possibilities of misdiagnosed cases. The ideal molecular diagnostic procedure should be highly sensitive and reliable as well as relatively cheap and cost-effective. PCR was first reported by Kary Mullis in 1985 for the amplification of individual target DNA segments in a genome.^{29,30} In 1988, a multiplex PCR that combined several primer pairs in the same reaction to amplify different specific amplicons was reported.³¹ The use of multiplex PCR is applicable to the detection of multiple amplicons, thus saving resources and substantially reducing turnaround time.³² In this study a multiplex PCR assay for the detection of HBs gene and human β -globin is characterized as a molecular diagnostic model with ICs. Findings are discussed.

2 | MATERIALS AND METHODS

2.1 | Cell culture

The human lung epithelial cell line A549 and hepatoma cell line Huh7 were a generous gift from Professor Mark Harris (University of Leeds, UK). Human embryonic kidney epithelial HEK293T and cervical

epithelial HeLa cell lines were a generous gift from Professor Nicola Stonehouse (University of Leeds, UK). Cells were maintained as monolayers in DMEM supplemented with 10% foetal bovine serum (FBS), 100 U/mL penicillin and 100 U/mL streptomycin. All cells were incubated at 37°C with 5% CO₂ and passaged upon confluence according to standard methods.³³

2.2 | DNA extraction

Cells were harvested at 80% confluency by trypsinisation with Trypsin EDTA. Total genomic DNA was extracted using TRIzol (phenol-chloroform method) following standard protocols.³⁴

2.3 | Plasmid clones

The HBsAg open reading frame flanked with NotI restriction sites and six base pairs (bp) linkers was synthesised commercially (Invitrogen, Thermo Fisher Scientific, Waltham, MA). The synthesized HBsAg gene was ligated into a *Stul*-linearized pCR-Blunt vector plasmid. The ligated plasmid was transformed into chemically competent *Escherichia coli* DH5 α cells and colonies screened by digestion with NotI. Nucleotide BLAST of all four cell line extracts matched NCBI reference human β -globin (NC_018922.2).³⁵

The human β -globin gene from A549 cells was amplified by PCR, purified by gel extraction and ligated into linearized pGEM T-easy plasmid vector (Life Technologies), following manufacturer's instructions. Plasmid vectors were then transformed into chemically competent *E. coli* DH5 α cells and colonies screened by digestion with EcoRI.

For quantitative analyses, plasmid copy number (PCN) was determined by standard methods.³⁶

2.4 | PCR reagents, primers, and thermocycling conditions

All PCR reactions were carried out using QIAGEN fast cycling PCR kit, following manufacturer's protocol. HBs gene was amplified using forward primer HBsAgF (5' GTAGTAGCCGCGCATGGAAGG-CAT) with reverse primer HBsAgR (5' TACATT-TAGCGGCCGCGTGTA). Human β -globin was amplified using modified GH20 upstream (5' GTAGTAGCGGCCGGAAGAGC-CAAGGACAGGTAC) and PC04 downstream (5' TAC-TACGCGGCCGCCCAACTTCATCCACGTTACC) primers.³⁷ PCR reactions were cycled as follows; one-cycle initial denaturation at 95°C for 1 min; 40 cycles of 5 s denaturation at 96°C, 5 s annealing at 55°C, and 1.75 min extension at 68°C. This was immediately followed by one cycle of final extension at 72°C for 1 min.

2.5 | Conventional PCR

Respective template PCN was determined as previously described. A set each of upstream and downstream HBs gene or β -globin primers was maintained at 0.5 μ M, for respective templates, in a 20 μ L

reaction. Thermocycling conditions were maintained as previously described.

2.6 | Mixed primer competition PCR

Template PCN was determined as previously described. Reactions were setup using increasing copies of β -globin or HBs gene templates. A set each of upstream and downstream HBs gene and β -globin primers was applied to final concentrations of 0.25 μ M for each primer in a 20 μ L reaction. Thermocycling conditions were maintained as previously described.

2.7 | Multiplex PCR

Template PCN was determined as previously described. Multiplex PCR was set up with increasing copies of β -globin and HBs gene plasmid templates (Table 1). Reactions were setup using upstream and downstream HBs gene and β -globin primers as previously described at a final concentration of 0.25 μ M for each primer in a 20 μ L reaction. Thermocycling conditions were maintained as previously described.

3 | RESULTS

3.1 | Generating control materials for PCR

The laboratory diagnose of clinical infections is more frequently employing molecular diagnostic techniques such as PCR. The use of IC in such techniques is essential for validating specimen quality and quantity, reducing the likelihood of false negative results. Targets typically used as ICs including HKG such as of β -globin, the abundance of which in mammalian cells is well characterized.^{10,11}

TABLE 1 Multiplex PCR template set up of HBsAg versus human β -globin plasmid copies

		Human β -globin plasmid copy (+)					
HBsAg plasmid copy (*)	0	+	++	+++	++++	+++++	+++++
	*	*	*	*	*	*	*
	**	+	++	+++	++++	+++++	+++++
	***	+	++	+++	++++	+++++	+++++
	****	+	++	+++	++++	+++++	+++++
	*****	+	++	+++	++++	+++++	+++++
	*****	+	++	+++	++++	+++++	+++++
	*****	+	++	+++	++++	+++++	+++++

Plasmid clones of HBsAg and human β -globin were added to multiplex PCR reactions at inversely proportional plasmid copies. Final primer concentrations of 0.25 μ M was maintained in each reaction. Table shows a checked board setup of PCR reactions in a 96-well plate. HBsAg plasmid copies are represented as asterisks (*), while human β -globin plasmid copies are presented as pluses (+).

In order to isolate the human β -globin gene to use as an IC in the molecular diagnosis of HBV in human samples, the total genomes were extracted from four human cell lines; Huh7, A549, HEK293T, and HeLa. The human β -globin gene was amplified from each cell extract, using target-specific modified PCR primers GH20 and PC04. The PCR amplicon from each cell line was gel-purified and sequenced. The nucleotide BLAST against known sequences showed a match (100 %) of all cell lines with the human chromosome 11 (from region 5226978 to 5227216), alternate assembly CHM1_1.1 (NCBI sequence ID: ref|NC_018922.2).³⁸ The purified PCR amplicon from cells was subsequently introduced into the cloning vector pGEM T-easy (Fig. 1A) to be employed in the downstream assays. The known sequence of the HBs gene was commercially synthesised as a blunt-ended DNA fragment and cloned into a *Stu*I-linearized pCR-Blunt vector plasmid (Fig. 1B) for downstream assays.

3.2 | Relative sensitivity of β -globin and HBs gene PCR

Stable plasmid clones containing the human β -globin or HBs gene allowed us to establish a controlled PCR for the detection of β -globin and HBs gene. In order to define the detection limits of these assays, respective PCR reactions were set up with a 10-fold serial dilution of HBs gene and human β -globin plasmid copies. PCR amplicons were separated through 2% agarose gel and product band intensities determined by densitometry (Fig. 2).

For the human β -globin PCR, product was clearly detected with 10^2 - 10^{11} genomes copies per reaction, with a linear range of 10^2 - 10^6 genome copies per reaction. In comparison, the PCR for HBs gene demonstrated a reduced linear range of 10^1 - 10^5 genome copies per reaction. These results may suggest a 10-fold greater sensitivity for HBs gene amplification under these PCR conditions compared to human β -globin, albeit with a reduced overall linear range.

3.3 | Mixed primers competition assays

Multiplex PCR employs multiple primer sets for the simultaneous amplification of multiple amplicons. However, the use of multiple primer sets in a single reaction can result in reduced specificity and sensitivity in comparison to single target PCR, partly due to the reduced primer concentration as well as primer dimerization, which can significantly reduce template-binding.³⁹ In order to address this, assays were designed to establish whether multiplex PCR conditions reduced the relative sensitivity of β -globin and HBs gene amplification.

Individual reactions were setup to amplify β -globin or HBs gene using multiplex PCR conditions and amplicons bands quantified by densitometry (Fig. 3). For both the β -globin and HBs gene multiplex PCR, products were detected with greater than 2.8×10^2 genome copies per reaction. This result would suggest that the multiplex reaction conditions reduced the sensitivity of HBs gene PCR approximately 10-fold, even in the absence of any β -globin or other competitive templates.

was observed. Like before, for the HBs gene under multiplex conditions in the absence of competing β -globin DNA (ie, 0 β -globin gene copy), products were only detected with greater than 2.8×10^2 genome copies per reaction. Upon addition of an increasing amount of competing β -globin DNA, a stepwise increase in product was observed even with below-detectable levels of HBs gene targets. This is indicative of non-specific amplification under multiplex PCR conditions when both target templates are present. Despite such, non-specific amplification, a linear increase in product was observed with greater than 2.8×10^2 HBs genome copies up to 2.8×10^4 copies per reaction. Therefore, after accounting for the non-specific amplification, the multiplex PCR can still be specifically detected above 2.8×10^2 HBs genome copies per reaction.

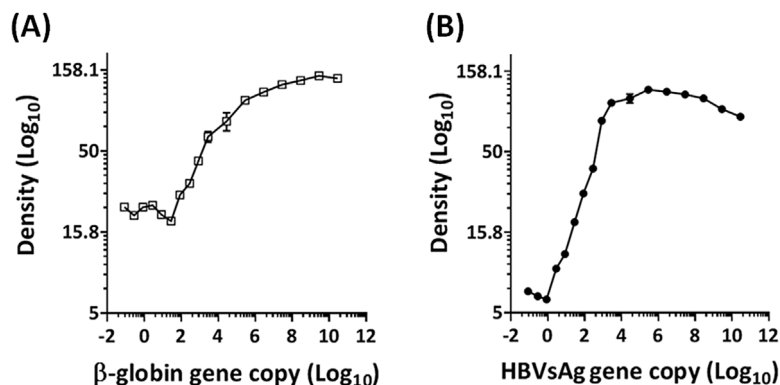


FIGURE 2 Input copy numbers assay showing densitometric plots of β -globin and HBs genes. In order to determine the linear ranges of conventional PCR for (A) β -globin and (B) HBs gene, the respective genes were amplified by PCR from a serial dilution of cloned targets with logarithmic increments in genome number. PCR amplicon was run through 2% agarose gel and DNA bands quantified by densitometry ($n = 2 \pm \text{S.E.M}$)

Similar results were observed for the detection of β -globin target under multiplex conditions, with an addition of increasing amount of competing DNA resulting in a stepwise increase in product observed with below-detectable levels of HBs of β -globin target gene. Again, such observations would be suggestive of non-specific amplification. However, an increase in PCR product was observed with greater than 2.8×10^2 of β -globin gene copies per reaction. Thus, the multiplex PCR can detect greater than 2.8×10^2 copies of β -globin DNA even under greater quantity of competing DNA. Therefore the multiplex PCR conditions can specifically detect both HBs and β -globin at greater than 2.8×10^2 DNA copies per reaction.

4 | DISCUSSION

The data suggests that PCR-amplification of HBs gene may be a highly sensitive and reliable means of diagnosing hepatitis. Serological detection of HBV infection is often applied to screening, diagnosis, and immuno-surveillance¹⁶ as an affordable option with a quick

turnaround time,^{42–44} however, it does not detect career status, levels of viremia, or chronicity. The supplementary detection of the HBVs gene may be more robust for diagnosis; to determine viral load, HBV genotype; to screen for anti-viral resistance, drug/therapeutic efficacy,⁴³ etc. Under conditions of conventional PCR, target genes are primed from single templates by a set of forward- and reverse-oriented gene-specific oligos, and amplified by a DNA polymerase in the presence of dNTPs. With these assays, 10 genomic copies of HBs gene were detectable with a single set of primers from a single template in a conventional PCR. Thus, as would be anticipated, amplification of parts or all of the HBV genome by conventional PCR is very specific with low detection limits.⁴³

The large difference in size between HBs gene and β -globin amplicons allowed for easy differentiation of both PCR products with these assays at varied primer concentrations. The ability to co-amplify templates within a single PCR reaction could significantly reduce diagnostic turnaround time especially in clinical settings. HKGs are indigenous and host-specific.²⁰ They are ideal quality indicators in medical diagnostics. The multiplex PCR conditions reduced PCR

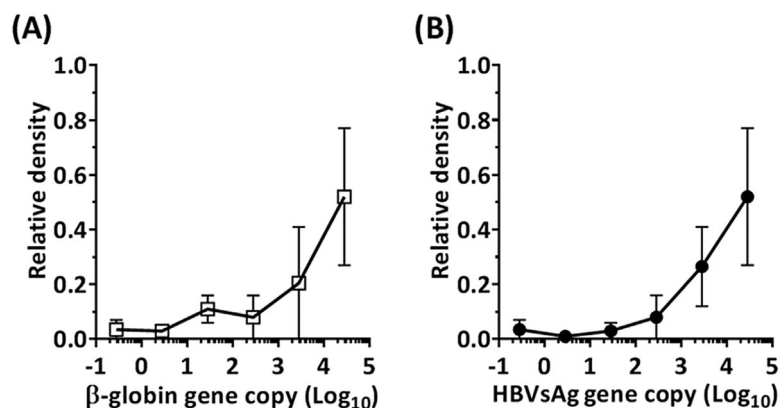


FIGURE 3 Mixed primers competition assays. To determine the effects of multiplex primers on PCR efficiency either (A) human β -globin or (B) HBsAg was amplified in a multiplex reaction containing equal concentrations of β -globin and HBsAg -specific primers. PCR products were analysed by agarose gel electrophoresis and DNA bands quantified by densitometry ($n = 2 \pm \text{S.E.M}$)

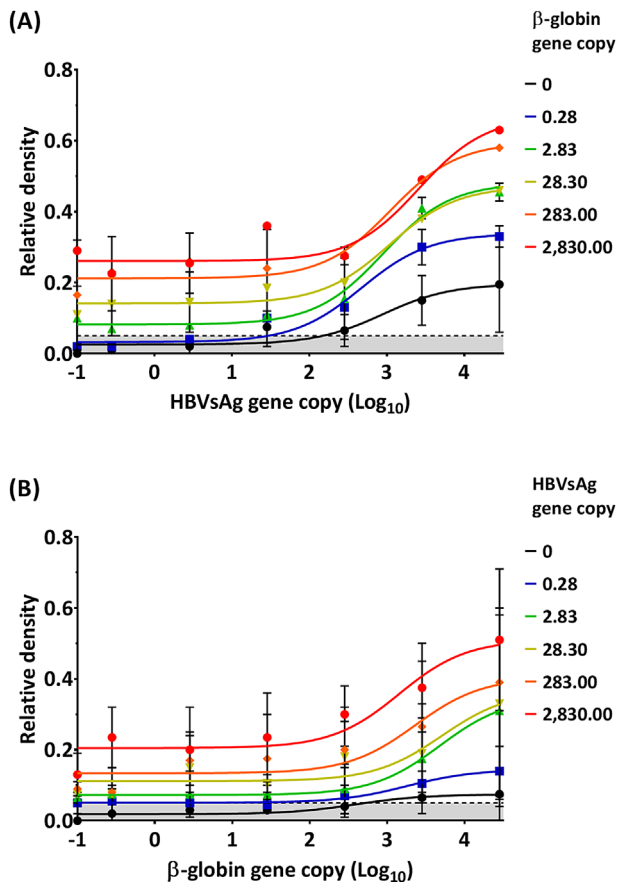


FIGURE 4 Multiplex PCR of β -globin and HBsAg with increasing genome copies. (A) Multiplex PCR of HBVsAg with increasing input copy number of β -globin. (B) Multiplex PCR of β -globin with increasing input copy number of HBVsAg. Both PCR amplicons were analysed by gel electrophoresis and DNA bands quantified by densitometry. A positive PCR was determined as having a relative density of above 0.05, based upon the data from the mixed primer competition assays. For clarity the area of the graph below 0.05 is shaded grey. ($n = 2 \pm \text{S.E.M}$)

sensitivity approximately 10-fold compared to conventional PCR, limiting the dynamic range from 2.8×10^2 up to 2.8×10^4 gene copies per reaction. This reduced dynamic range could suggest that a limited serial dilution of sample may be required for semi-quantitative diagnostic purposes. Under conditions where both PCR targets are present, the sensitivity of the multiplex PCR did not appear to change significantly. However, the specificity of the multiplex PCR was reduced with some non-specific amplification observed in the presence of high concentration of non-target DNA.

The multiplex assays suggest that, at optimal priming conditions, co-amplifying β -globin together with the gene of interest (eg HBs DNA) integrates a standard qualitative sample-based positive control, as an alternative to multiple PCR reactions, thereby avoiding risks of contamination. However these advantages come at the cost of a slightly reduced sensitivity, and importantly reduced specificity. This latter limitation could however be potentially accounted for by performing a small limiting dilution alongside standardized dilution

series of β -globin and HBs target DNA clones. Furthermore, a dilution series of β -globin could be used to generate an ideal standard curve to quantitatively assess abundance of template in the sample.

In the laboratory diagnosis of HBV, PCR has been shown to have very high sensitivity and specificity.¹⁶ In this study, the sensitivity,²² of conventional PCR was observed to be higher than the multiplex PCR assays and multi-primer competition PCR. This strengthens the submission that PCR efficiency is dependent on amounts of available primers and if they are in excess.⁴⁵ It further suggests that assay multiplex PCR assay could be ideal for multiple template amplification within a single reaction.

5 | CONCLUSION

These findings suggest detection limits of less than 10 genome copies of either template in conventional and multiplex PCR conditions. With the use of multi-primer sets for the amplification of single and multi-template samples, these findings show that not only are ICs good indicators of quality assurance of sample processing, co-amplification of IC with gene of interest (HBs) may have a resultant effect on the viability of the chosen assay. If fully optimized, this assay would provide a diagnostic complement to serological diagnosis and/or screening of HBV thus providing a semi-quantitative measurement of viral load. Such assays have been applied to diagnose multiple of organisms⁴⁶ or conditions from limited clinical samples within a single reaction.

ACKNOWLEDGEMENT

The authors would like to thank Professors N.J. Stonehouse and D.J. Rowlands for accommodating the study. This work was supported by the Tertiary Education Trust Fund (TETFund), Nigeria [grant number, TETFund/DESS/NRF/20/13/STI/VOL.1] and carried out in collaboration with the Stonehouse group at the School of Molecular and Cellular Biology, Faculty of Biological Sciences, University of Leeds, UK.

AUTHORS' CONTRIBUTIONS

OOA conceived the study; OOA and MRH designed the study protocol; OOA carried out all experiments; OOA and MRH analyzed and interpreted the data. All authors drafted the manuscript. All authors critically revised the manuscript for intellectual content. All authors read and approved the final manuscript.

CONFLICTS OF INTEREST

None declared.

REFERENCES

- Goldstein ST, Zhou F, Hadler SC, et al. A mathematical model to estimate global hepatitis B disease burden and vaccination impact. *Int J Epidemiol.* 2005;34:1329–1339.

2. Zanetti AR, Van Damme P, Shouval D. The global impact of vaccination against hepatitis B: a historical overview. *Vaccine*. 2008;26:6266–6273.
3. Kao JH, Chen DS. Global control of hepatitis B virus infection. *Lancet Infect Dis*. 2002;2:395–403.
4. Publication, W.H.O. Hepatitis B vaccines: WHO position paper—recommendations. *Vaccine*. 2010;28:589–590.
5. Lau JY, Wright TL. Molecular virology and pathogenesis of hepatitis B. *Lancet*. 1993;342:1335–1340.
6. Kramvis A, Kew M, Francois G. Hepatitis B virus genotypes. *Vaccine*. 2005;23:2409–2423.
7. Hayer J, Jadeau F, Deleage G, Kay A, Zoulim F, Combet C. HBVdb: a knowledge database for hepatitis B virus. *Nucleic Acids Res*. 2013;41:D566–D570.
8. Tran TT, Trinh TN, Abe K. New complex recombinant genotype of hepatitis B virus identified in Vietnam. *J Virol*. 2008;82:5657–5663.
9. Tatematsu K, Tanaka Y, Kurbanov F, et al. A genetic variant of hepatitis B virus divergent from known human and ape genotypes isolated from a Japanese patient and provisionally assigned to new genotype J. *J Virol*. 2009;83:10538–10547.
10. Lanford RE, Chavez D, Brasky KM, Burns RB, 3rd, Rico-Hesse R. Isolation of a hepadnavirus from the woolly monkey, a New World primate. *Proc Natl Acad Sci USA*. 1998;95:5757–5761.
11. Vaudin M, Wolstenholme AJ, Tsiquaey KN, Zuckerman AJ, Harrison TJ. The complete nucleotide sequence of the genome of a hepatitis B virus isolated from a naturally infected chimpanzee. *J Gen Virol*. 1988;69:1383–1389.
12. Warren KS, Heeney JL, Swan RA, Heriyanto, Verschoor EJ. A new group of hepadnaviruses naturally infecting orangutans (*Pongo pygmaeus*). *J Virol*. 1999;73:7860–7865.
13. Summers J, Smolec JM, Snyder R. A virus similar to human hepatitis B virus associated with hepatitis and hepatoma in woodchucks. *Proc Natl Acad Sci USA*. 1978;75:4533–4537.
14. Marion PL, Oshiro LS, Regnery DC, Scullard GH, Robinson WS. A virus in beechey ground-squirrels that is related to hepatitis-B virus of humans. *Proc Natl Acad Sci USA*. 1980;77:2941–2945.
15. Mason WS, Seal G, Summers J. Virus of Pekin ducks with structural and biological relatedness to human hepatitis B virus. *J Virol*. 1980;36:829–836.
16. Krajden M, McNabb G, Petric M. The laboratory diagnosis of hepatitis B virus. *Can J Infect Dis Med Microbiol*. 2005;16:65–72.
17. Kao JH. Diagnosis of hepatitis B virus infection through serological and virological markers. *Expert Rev Gastroenterol Hepatol*. 2008;2:553–562.
18. Heermann KH, Gerlich WH, Chudy M, Schaefer S, Thomssen R, Group TEP. Quantitative detection of hepatitis B virus DNA in two international reference plasma preparations. Eurohep Pathobiology Group. *J Clin Microbiol*. 1999;37:68–73.
19. Dheda K, Huggett JF, Bustin SA, Johnson MA, Rook G, Zumla A. Validation of housekeeping genes for normalizing RNA expression in real-time PCR. *Biotechniques*. 2004;37:112–114.
20. Eisenberg E, Levanon EY. Human housekeeping genes, revisited (vol 29, pg 569, 2013). *Trends Genet*. 2014;30:119–120.
21. Akobeng AK. Understanding diagnostic tests 1: sensitivity, specificity and predictive values. *Acta Paediatrica*. 2007;96:338–341.
22. Smith CJ. Diagnostic tests (1) – sensitivity and specificity. *Phlebology*. 2012;27:250–251.
23. Zampino R, Boemio A, Sagnelli C, et al. Hepatitis B virus burden in developing countries. *World J Gastroenterol*. 2015;21:11941–11953.
24. Stabinski L, O'Connor S, Barnhart M, Kahn RJ, Hamm TE. Prevalence of HIV and hepatitis B virus co-infection in sub-Saharan Africa and the potential impact and program feasibility of hepatitis B surface antigen screening in resource-limited settings. *J Acquir Immune Defic Syndr*. 2015;68:S274–S285.
25. Afzali H, Momen Heravi M, Moravveji SA, Poorrahnama M. Prevalence of hepatitis B surface antigen in pregnant women in beheshti hospital of kashan, isfahan. *Iran Red Crescent Med J*. 2015;17:e20598.
26. Adegbesan-Omilabu M, Okunade K, Gbadegesin A, Olowoselu O, Oluwole A, Omilabu S. Seroprevalence of hepatitis B virus infection among pregnant women at the antenatal booking clinic of a Tertiary Hospital in Lagos Nigeria. *Niger J Clin Pract*. 2015;18:819–823.
27. Olokoba A, Salawu F, Danburam A, et al. Hepatitis B virus infection amongst pregnant women in North-Eastern Nigeria- A call for action. *Niger J Clin Pract*. 2011;14:10–13.
28. Musa BM, Bussell S, Borodo MM, Samaila AA, Femi OL. Prevalence of hepatitis B virus infection in Nigeria, 2000–2013: A systematic review and meta-analysis. *Niger J Clin Pract*. 2015;18:163–172.
29. Mullis K, Faloona F, Scharf S, Saiki R, Horn G, Erlich H. Specific enzymatic amplification of DNA in vitro: the polymerase chain reaction. *Cold Spring Harb Symp Quant Biol*. 1986;51:263–273.
30. Saiki RK, Scharf S, Faloona F, et al. Enzymatic amplification of beta-globin genomic sequences and restriction site analysis for diagnosis of sickle cell anemia. *Science*. 1985;230:1350–1354.
31. Chamberlain JS, Gibbs RA, Ranier JE, Nguyen PN, Caskey CT. Deletion screening of the Duchenne muscular dystrophy locus via multiplex DNA amplification. *Nucleic Acids Res*. 1988;16:11141–11156.
32. Markoulatos P, Sifakas N, Moncany M. Multiplex polymerase chain reaction: a practical approach. *J Clin Lab Anal*. 2002;16:47–51.
33. Masters JR, Stacey GN. Changing medium and passaging cell lines. *Nat Protoc*. 2007;2:2276–2284.
34. Chomczynski P. A reagent for the single-Step simultaneous isolation of rna, DNA and proteins from cell and tissue samples. *Biotechniques*. 1993;15:532–534.
35. Taylor TD, Noguchi H, Totoki Y, et al. Human chromosome 11 DNA sequence and analysis including novel gene identification. *Nature*. 2006;440:497–500.
36. Cooper NS, Brown ME, Caulcott CA. A mathematical method for analysing plasmid stability in micro-organisms. *J Gen Microbiol*. 1987;133:1871–1880.
37. Resnick RM, Cornelissen MTE, Wright DK, et al. Detection and typing of human papillomavirus in archival cervical-Cancer specimens by DNA amplification with consensus primers. *J Natl Cancer Inst*. 1990;82:1477–1484.
38. Lowe TM, Eddy SR. TRNAscan-SE: A program for improved detection of transfer RNA genes in genomic sequence. *Nucleic Acids Res*. 1997;25:955–964.
39. Brownie J, Shawcross S, Theaker J, et al. The elimination of primer-dimer accumulation in PCR. *Nucleic Acids Res*. 1997;25:3235–3241.
40. Gong R, Li SY. Extraction of human genomic DNA from whole blood using a magnetic microsphere method. *Int J Nanomedicine*. 2014;9:3781–3788.
41. Banda M, Bommineni A, Thomas RA, Luckinbill LS, Tucker JD. Evaluation and validation of housekeeping genes in response to ionizing radiation and chemical exposure for normalizing RNA expression in real-time PCR. *Mutat Res*. 2008;649:126–134.
42. Wu X, Zhou C, Huang WJ, et al. [Sensitivity and specificity of 4 domestic ELISA kits for detection of hepatitis B virus markers]. *Zhonghua Liu Xing Bing Xue Za Zhi*. 2008;29:915–918.
43. Villar LM, Cruz HM, Barbosa JR, Bezerra CS, Portilho MM, Scalioni Lde P. Update on hepatitis B and C virus diagnosis. *World J Virol*. 2015;4:323–342.
44. Ba Alawi F, Robertson PW, LePage AK, Jayamaha J, Baleriola C, Rawlinson WD. The reliability of HBV core antibody in serological screening for hepatitis B virus. *Pathology*. 2013;45:501–505.
45. Lorenz TC. Polymerase chain reaction: basic protocol plus troubleshooting and optimization strategies. *J Vis Exp*. 2012;63:3998.

46. Binnicker MJ. Multiplex molecular panels for diagnosis of gastrointestinal infection: performance, result interpretation, and cost-effectiveness. *J Clin Microbiol.* 2015;53:3723–3728.
47. Saiki RK, Gelfand DH, Stoffel S, et al. Primer-directed enzymatic amplification of DNA with a thermostable DNA-Polymerase. *Science.* 1988;239:487–491.
48. Coutlee F, Gravitt P, Richardson H, et al. Nonisotopic detection and typing of human papillomavirus DNA in genital samples by the line blot assay. *J Clin Microbiol.* 1999;37:1852–1857.

How to cite this article: Adeyemi OO, Herod MR, Oladiji F, Fakunle YM, Babatunde AS, Agbede OO. A multi-template multiplex PCR assay for hepatitis B virus and human β -globin. *J Med Virol.* 2017;89:1944–1951.
<https://doi.org/10.1002/jmv.24877>